



**South Carolina State Ports  
Authority – Continuous Air  
Monitoring Station for the Wando  
Welch Terminal**

Quarterly Report

October 2011



**South Carolina State Ports  
Authority - Continuous Air  
Monitoring Station for the  
Wando Welch Terminal**

Quarterly Report

Prepared for:

South Carolina State Ports Authority  
176 Concord Street  
Charleston  
South Carolina 29401

Prepared by:

ARCADIS U.S., Inc.  
4915 Prospectus Drive  
Suite F  
Durham  
North Carolina 27713  
Tel 919 544 4535  
Fax 919 544 5690

Our Ref.:

RN006310

Date:

October 2011

*This document is intended only for the use of the individual or entity for which it was prepared and may contain information that is privileged, confidential and exempt from disclosure under applicable law. Any dissemination, distribution or copying of this document is strictly prohibited.*

<b>1. Introduction</b>	<b>1</b>
1.1 Scope	1
1.2 Project Description	1
<b>2. Quarterly Results</b>	<b>2</b>
2.1 Specific Data Notes	8
<b>3. Quality Assurance/Quality Control</b>	<b>8</b>
3.1 Daily QC/Validation	8
3.2 Quarterly Data Validation	8

**Tables**

Table 2-1.	24-Hour Averages	2
Table 2-2.	Quarterly Statistics	5
Table 2-3.	Monthly Statistics	7

**Figures**

Figure 2-1.	24-hour Averages	6
Figure 2-2.	Max 1-hour Averages	7

**Appendices**

A	Quality Assurance Project Plan for Continuous Air Monitoring Station for the Wando Welch Terminal	
---	---	--

## **1. Introduction**

### **1.1 Scope**

ARCADIS U.S., Inc. (ARCADIS) was contracted in late December 2010 to provide Continuous Air Monitoring Services to the South Carolina State Ports Authority (SCSPA) at the Wando Welch Terminal in Charleston. ARCADIS has followed through on the planned schedule and activities since that award. The major accomplishments were to complete the Quality Assurance Plan (QAP), purchase the instruments, complete the site setup, and then to begin acquiring the data. This report begins the submittal of quarterly data reports and presents the data summaries requested by SCSPA and described in the work scope. The data acquisition was started on May 6, 2011 in line with the court mandated start date. This report encompasses a period corresponding to data taken during the period from July 1, 2011 through September 30, 2011.

### **1.2 Project Description**

SCSPA asked for technical support that will provide ambient air quality data including particulate matter less than 2.5 microns ( $PM_{2.5}$ ),  $SO_2$ , and  $NO_2$  for a period of 5 years at the Wando Welch Terminal of the port of Charleston. ARCADIS will maintain the monitoring instruments, stock consumables such as filters and calibration gases, and order spare parts such that downtime will be avoided. ARCADIS has established standard operating procedures to perform daily downloads and to provide Level 1 data validation for the resulting data. This monitoring project setup was relatively straightforward and has proven to be reliable and is generating valid high quality data suitable for use in dispersion modeling or other potential purposes.

As required, periodically the QAP and procedures are updated to reflect improvements to the basic operating procedures. This QAP is written consistent with the current ambient air quality standards for PM,  $NO_x$  and  $SO_2$  as defined by the U.S. Environmental Protection Agency. Excursions beyond these standards have not been seen, but a few daily spikes and rises have been noted and correlating local conditions are investigated in local media outlets and recorded when seen. These observations are tabulated and presented in the quarterly reports.

The location selected for sampling and the sampling equipment has proven to be well-suited for the project as it is centrally located to the port activities and has proven to be very responsive to local equipment air emissions and the local meteorological

conditions. Although this is not a typical fence line site, it has shown high value in permitting the evaluation of port activities and related air quality effects. We have been able to remotely access the control computer and reliably interact with the instruments. We can see immediate reaction from the instruments in response to events such as container handling equipment and the morning openings of the front gates to entering truck traffic. These patterns can be reviewed in details in the archived data any time in the future if needed.

## 2. Quarterly Results

The 24-hr daily averages for PM, NO, NO<sub>2</sub>, NO<sub>x</sub>, and SO<sub>2</sub> and the maximum daily value (1-hr average) for NO<sub>2</sub> and SO<sub>2</sub> for this period are shown in Table 2-1. The red highlighted cells indicate exceedances. Quarterly statistics showing the averages, minimums and maximums for all parameters are summarized in Table 2-2. 24-hr averages for all constituents are also shown graphically in Figure 2-1. Maximum 1-hr averages for NO<sub>2</sub> and SO<sub>2</sub> are shown in Figure 2-2. Statistics are broken down by months and summarized in Table 2-3.

**Table 2-1. 24-Hour Averages**

Date	24-hour Averages					Daily Max 1-hr Avg.	
	PM ( $\mu\text{g}/\text{m}^3$ )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> ppb)	SO <sub>2</sub> (ppb)
7/1/11	22.92	1.51	3.17	4.60	0.82	10.10	6.21
7/2/11	10.79	0.11	0.11	0.20	0.04	1.34	0.63
7/3/11	8.19	0.08	0.06	0.11	0.05	0.41	0.71
7/4/11	10.92	0.00	0.00	0.00	0.03	0.02	0.34
7/5/11	14.01	5.53	3.09	8.44	1.50	11.95	12.10
7/6/11	11.31	6.36	1.58	7.49	0.03	5.86	0.42
7/7/11	7.82	7.36	2.14	9.08	0.20	6.93	2.05
7/8/11	6.80	7.27	2.94	10.00	1.58	14.63	16.18
7/9/11	11.89	0.17	0.31	0.44	0.30	1.88	3.42
7/10/11	18.37	0.01	0.03	0.03	0.02	0.27	0.29
7/11/11	38.16	5.32	4.36	9.57	0.05	13.51	0.23
7/15/11	11.56	0.33	1.13	1.42	0.00	8.56	0.00
7/16/11	12.63	0.00	0.00	0.00	0.00	0.00	0.00
7/17/11	12.31	0.00	0.00	0.00	0.05	0.00	0.12



Date	24-hour Averages					Daily Max 1-hr Avg.	
	PM ( $\mu\text{g}/\text{m}^3$ )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> ppb)	SO <sub>2</sub> (ppb)
7/18/11	5.74	3.47	1.74	4.93	0.15	10.18	0.56
7/19/11	19.68	1.05	3.63	4.67	1.10	16.42	3.52
7/20/11	16.01	4.10	9.84	13.93	1.49	27.24	7.71
7/21/11	21.80	4.35	10.04	14.38	0.79	26.77	3.78
7/22/11	8.96	0.10	1.99	2.08	0.02	2.73	0.03
7/25/11	11.51	7.99	7.18	15.17	23.27	15.39	-----
7/26/11	9.93	7.61	8.77	16.37	2.54	19.39	18.31
7/27/11	9.47	7.23	7.15	14.37	6.22	16.78	-----
7/28/11	10.02	5.36	6.12	11.46	20.95	13.15	-----
7/29/11	13.23	6.74	7.15	13.87	2.70	13.92	11.92
7/30/11	14.62	0.50	4.26	4.75	0.61	14.34	5.33
7/31/11	12.26	0.43	11.35	11.77	0.08	-----	1.42
8/1/11	10.73	4.19	13.69	17.80	0.34	36.73	6.90
8/2/11	20.54	3.13	11.91	15.04	1.70	26.74	7.32
8/3/11	14.14	3.97	8.63	12.59	1.22	19.68	7.13
8/4/11	17.78	3.27	6.93	10.18	0.64	20.10	2.30
8/5/11	12.27	5.24	6.91	12.13	0.24	22.91	2.99
8/6/11	9.71	0.32	1.63	1.88	0.48	11.38	6.90
8/7/11	11.95	0.28	0.59	0.85	0.73	5.66	5.17
8/8/11	17.77	2.02	5.07	7.07	0.41	14.00	2.47
8/9/11	9.01	4.61	10.06	14.62	7.08	22.94	18.58
8/10/11	13.79	5.26	11.87	17.11	3.38	22.19	11.79
8/11/11	14.65	4.30	10.38	14.64	1.74	22.85	7.52
8/12/11	14.09	3.91	7.78	11.66	0.08	27.93	0.85
8/13/11	6.64	0.01	0.63	0.61	0.04	3.81	0.67
8/14/11	8.81	0.10	1.89	1.91	0.31	6.15	2.39
8/15/11	14.06	4.46	11.40	15.82	3.86	23.70	16.15
8/16/11	16.82	2.68	9.11	11.72	0.50	22.97	2.61
8/17/11	12.96	1.43	5.50	6.87	0.06	19.48	0.46
8/18/11	21.41	2.71	4.99	7.66	0.09	16.19	1.30



**SCSPA - Continuous  
Air Monitoring Station  
for the Wando Welch  
Terminal**

Q3 2011 Report

Date	24-hour Averages					Daily Max 1-hr Avg.	
	PM ( $\mu\text{g}/\text{m}^3$ )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> ppb)	SO <sub>2</sub> (ppb)
8/19/11	10.85	3.94	7.85	11.77	0.77	24.55	4.22
8/20/11	11.17	0.08	0.65	0.69	0.41	2.57	2.02
8/21/11	13.83	0.29	0.51	0.79	0.18	4.37	0.77
8/22/11	19.07	4.89	8.35	13.20	2.52	23.41	10.60
8/23/11	12.94	4.54	8.33	12.81	0.55	27.91	5.03
8/24/11	7.35	4.05	8.24	12.27	0.07	19.88	1.19
8/25/11	12.20	4.10	3.74	7.78	0.02	14.40	0.50
8/26/11	6.01	1.22	0.94	2.15	0.05	4.65	0.54
8/27/11	13.16	1.30	2.20	3.48	2.81	8.22	14.36
8/28/11	17.36	0.11	1.36	1.38	0.66	4.35	2.83
8/29/11	25.32	7.29	8.56	15.80	0.24	30.98	1.36
8/30/11	12.32	2.26	3.98	6.19	0.05	11.02	0.97
8/31/11	10.54	1.83	2.88	4.69	0.02	8.91	0.33
9/1/11	9.36	2.68	6.27	8.91	0.02	13.80	0.20
9/2/11	10.02	3.01	8.42	11.38	0.62	27.58	2.89
9/3/11	3.69	0.09	0.96	1.00	0.17	4.40	1.10
9/4/11	8.62	0.03	1.22	1.20	0.01	11.70	0.21
9/5/11	4.95	0.00	0.14	0.13	0.06	2.01	0.95
9/6/11	7.76	6.37	4.73	11.07	0.39	10.99	7.27
9/7/11	6.07	8.32	10.82	19.08	2.83	20.19	15.04
9/8/11	10.65	7.58	10.90	18.45	2.27	22.78	12.41
9/9/11	12.77	6.98	9.48	16.41	2.21	23.50	12.56
9/10/11	12.80	0.23	2.37	2.53	1.10	11.11	2.83
9/11/11	14.01	0.67	2.95	3.59	0.25	14.08	1.38
9/12/11	8.03	10.10	11.22	21.28	2.00	25.87	18.90
9/13/11	7.09	14.12	11.77	25.83	0.24	25.48	2.28
9/14/11	9.92	6.70	10.09	16.75	0.06	32.16	0.48
9/15/11	17.46	10.78	12.36	23.11	0.73	34.19	6.85
9/16/11	7.11	3.43	3.25	6.64	0.04	8.10	0.85
9/17/11	9.73	0.22	1.12	1.28	0.02	2.65	0.17



24-hour Averages						Daily Max 1-hr Avg.	
Date	PM ( $\mu\text{g}/\text{m}^3$ )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> (ppb)	SO <sub>2</sub> (ppb)
9/18/11	4.50	0.01	0.00	0.01	0.00	0.01	0.12
9/19/11	6.26	1.90	2.07	3.97	0.01	8.27	0.15
9/20/11	7.51	2.68	3.52	6.18	0.01	11.26	0.31
9/21/11	6.10	9.23	7.34	16.53	0.05	21.09	0.42
9/22/11	4.21	6.35	6.56	12.89	0.09	14.64	1.49
9/23/11	6.52	8.53	6.47	14.97	0.40	18.67	3.20
9/24/11	2.73	0.11	0.59	0.66	0.04	4.60	0.95
9/25/11	3.88	0.01	0.01	0.01		0.10	0.49
9/26/11	3.81	12.62	5.91	18.47	0.04	19.97	0.77
9/27/11	3.93	8.48	6.72	15.14	0.49	19.56	3.04
9/28/11	12.48	7.79	9.24	17.00	0.54	25.16	2.46
9/29/11	12.51	8.83	11.71	20.50	3.04	25.60	8.83
9/30/11	10.66	8.20	13.60	21.76	6.72	32.33	26.48

\* Red cells indicate exceedances

----- Due to calibration system malfunctions, data is unavailable

Table 2-2. Quarterly Statistics

24-hour Averages						Daily Max 1-hr Avg.	
Date	PM ( $\mu\text{g}/\text{m}^3$ )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> (ppb)	SO <sub>2</sub> (ppb)
Average	11.67	3.76	5.36	9.07	1.38	15.12	4.51
Minimum	2.73	0.00	0.00	0.00	0.00	0.00	0.00
Maximum	38.16	14.12	13.69	25.83	23.27	36.73	26.48




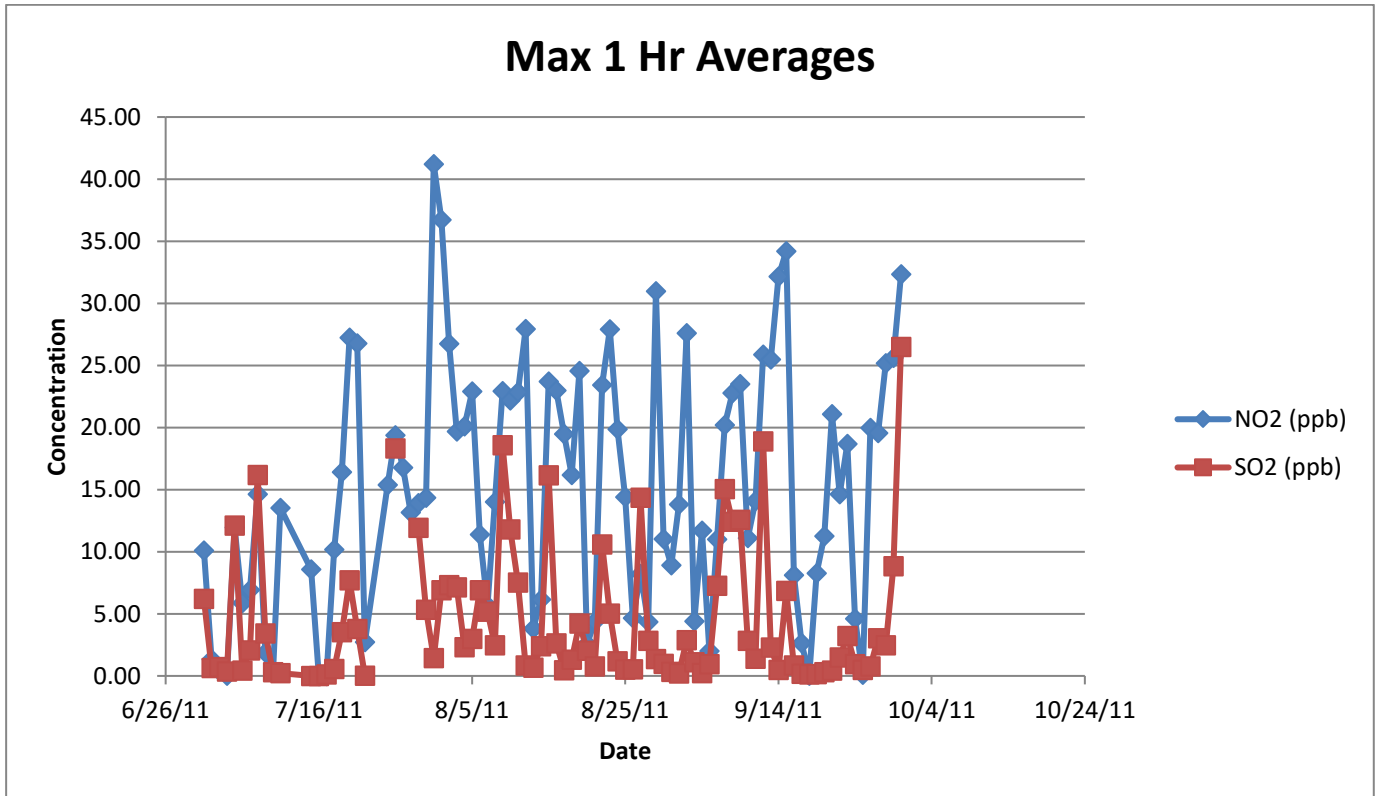


Figure 2-1. 24-hour Averages



**Figure 2-2. Max 1-hour Averages**

**Table 2-3. Monthly Statistics**

Month	Monthly Averages					Monthly Daily Max 1-hr Avg.	
	PM (µg/m <sup>3</sup> )	NO (ppb)	NO <sub>2</sub> (ppb)	NO <sub>x</sub> (ppb)	SO <sub>2</sub> (ppb)	NO <sub>2</sub> (ppb)	SO <sub>2</sub> (ppb)
July 2011	13.50	3.19	3.77	6.89	2.48	10.07	4.14
August 2011	13.52	2.83	6.02	8.81	1.01	17.12	4.78
September 2011	8.17	5.20	6.06	11.22	0.82	16.40	4.50

## 2.1 Specific Data Notes

During July, there were several periods of monitoring failure that required specific diagnostic actions and an investigation. These issues were identified and addressed. Normal operations returned by early August.

## 3. Quality Assurance/Quality Control

QA/QC procedures applied to this project are described in a Quality Assurance Project Plan titled *Continuous Air Monitoring Station for the Wando Welch Terminal* (July 8, 2011)

### 3.1 Daily QC/Validation

According to the QAP prepared for this work, results were reviewed for anomalies and validated on a daily basis. These validations were recorded on QA/QC Daily Comment Sheets. Exceedances of the EPA Ambient Air Quality guidelines found in the daily validations were logged and are summarized in Table 3-1. The table contains the date the anomaly occurred and the reason/comment.

**Table 3-1. QA/QC Daily Comment Sheet**

Date	Comment
7/11/2011 – 7/18/2011	System down intermittently for maintenance issues
7/25/2011 – 7/28/2011	Failures during SO <sub>2</sub> instrument calibrations
7/31/2011	Extended NO <sub>2</sub> calibration failures
8/01/2011	The calibration system problem resolved by modifying the heated sample line

### 3.2 Quarterly Data Validation

The quarterly data were assessed as follows: 100% of the validated Quarter 3 data were flagged as “good”. Percent completeness for Quarter 3 was calculated by dividing the number of hours flagged by the macro as “Insufficient Data” for any parameter by the total number of hours in the quarter. Percent completeness for Quarter 3 was 89.76%.



**SCSPA - Continuous  
Air Monitoring Station  
for the Wando Welch  
Terminal**

Q3 2011 Report